Experiment HH-11: ECG ~ Simulations and Comparisons

Equipment Required

PC or Mac Computer

IXTA, USB cable, IXTA power supply

ROAM ECG

ECG-SIM files

Alcohol swabs

Disposable ECG electrodes

ROAM Setup

1. For this lab – leave the ROAM in the dock.

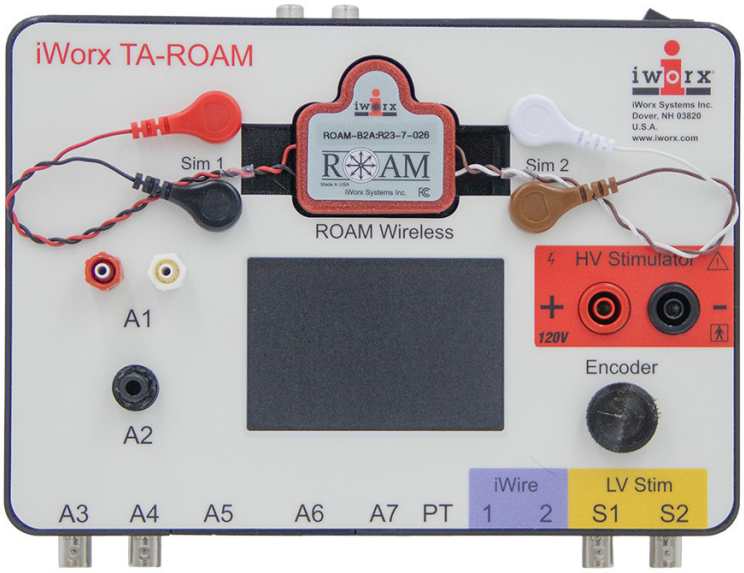

Figure HH-11-S1: The TA with the ROAM in the dock.

Lab

How to Use the Simulator Files

1. Click the drop down next to **Simulator**
2. Choose the cardiac simulation you wish to run.
3. Click Record.
4. The simulation will record for 30 seconds.
5. Repeat for any of the ECG Sim files.

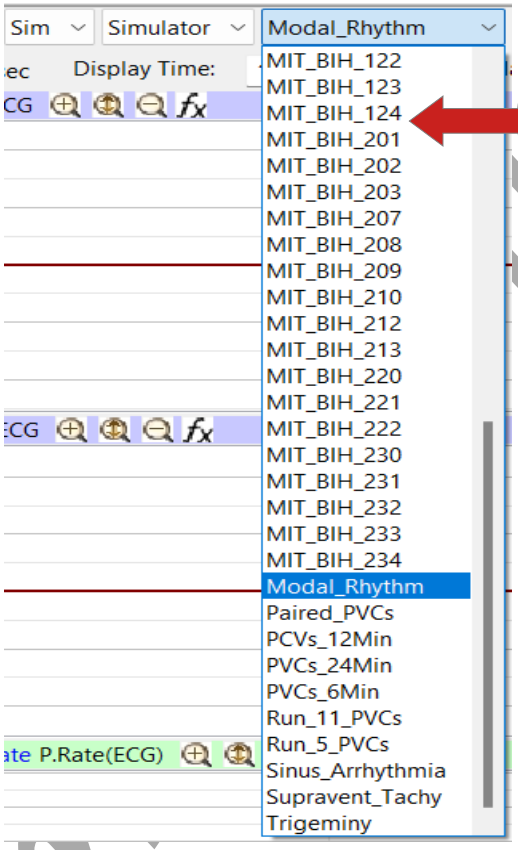

Iworx Sample